


INDIVIDUAL THICKNESS VARIATION RECORD

Test No. _____

Product Name	CEFUROXIME AXETIL IP 500 MG		
Batch No.	BVK65895S	Department	Production
BFG Code No.	BFG-112030	Date	24.04.2026
No. of Samples	50	Start Time	15:08:50
Equipment Code No.	EQP-15552	Vernier Code No.	M/VC-28
Standard Thickness (mm)	10.00	Side	NA / LHS / RHS
Std. Lower Limit (mm)	8.00	Std. Upper Limit (mm)	12.00

Test Results

Average Thickness (mm)	10.86	Standard Deviation	0.3200
Minimum Thickness (mm)	10.25	No. of Tablets Below Limit	0
Maximum Thickness (mm)	11.50	No. of Tablets Above Limit	0

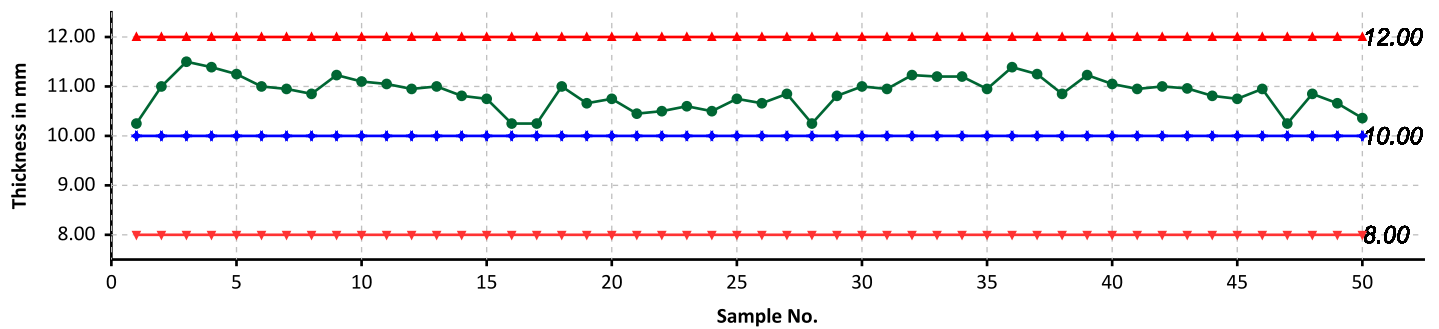

—●— Actual Value
 —▲— Upper
 —▼— Lower
 —◆— Standard

Sample No.	Thickness (mm)	Sample No.	Thickness (mm)	Sample No.	Thickness (mm)	Sample No.	Thickness (mm)	Sample No.	Thickness (mm)
1	10.25	2	11.00	3	11.50	4	11.39	5	11.25
6	11.00	7	10.95	8	10.85	9	11.23	10	11.10
11	11.05	12	10.95	13	11.00	14	10.81	15	10.75
16	10.25	17	10.25	18	11.00	19	10.66	20	10.75
21	10.45	22	10.50	23	10.60	24	10.50	25	10.75
26	10.66	27	10.85	28	10.25	29	10.81	30	11.00
31	10.95	32	11.23	33	11.20	34	11.20	35	10.95
36	11.39	37	11.25	38	10.85	39	11.23	40	11.05
41	10.95	42	11.00	43	10.96	44	10.81	45	10.75
46	10.95	47	10.25	48	10.85	49	10.66	50	10.36

Result: Complies

Done by : Mangesh Rane

Date : 24.04.2026