




HARDNESS & DIMENSION REPORT

Test No. _____

Product Name	TOPIRAMATE 200MG TABLETS USP		
Batch No.	BV3242342	Department	Production
BFG Code No.	BFG-12030	Date	27.04.2026
No. of Samples	20	Start Time	15:14:34
Equipment Code No.	SG-136	Hardness Tester Code No.	HD-425
Side	NA / LHS / RHS		

Standard Limits

Hardness (N)		Thickness (mm)		Length(mm)	
Lower =	50	Lower =	8.00	Lower =	10.00
Standard =	75	Standard =	10.00	Standard =	12.00
Upper =	100	Upper =	12.00	Upper =	14.00

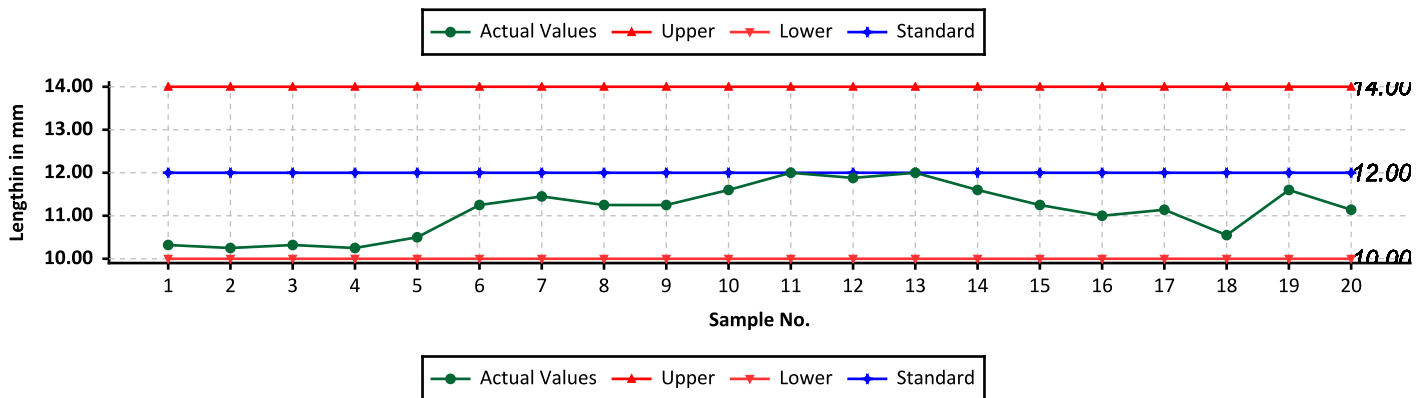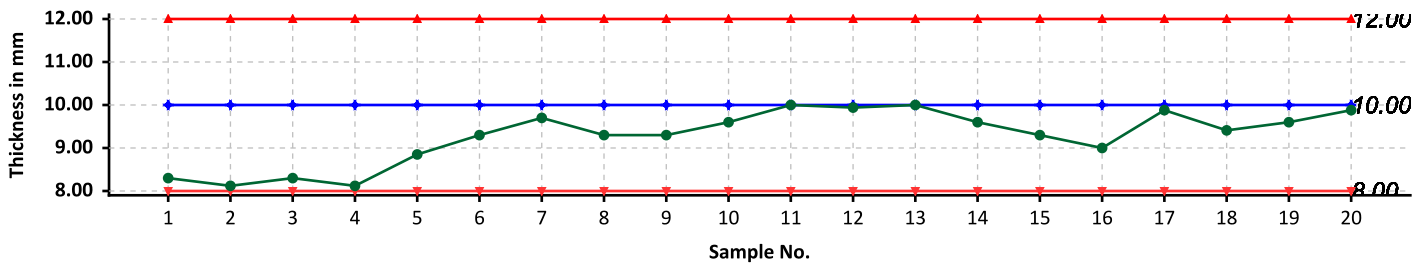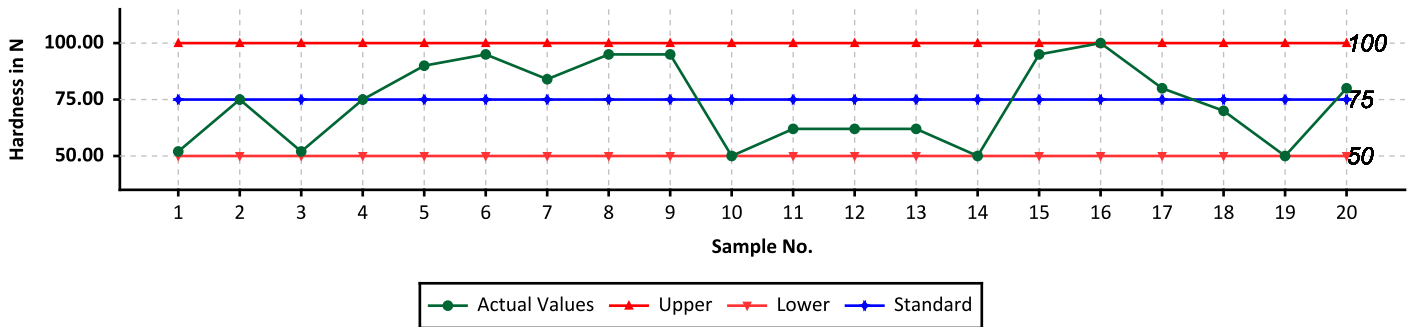

HARDNESS & DIMENSION REPORT

Test Results			
Sample No.	Hardness (N)	Thickness (mm)	Length (mm)
1	52	8.30	10.32
2	75	8.12	10.25
3	52	8.30	10.32
4	75	8.12	10.25
5	90	8.85	10.50
6	95	9.30	11.25
7	84	9.70	11.45
8	95	9.30	11.25
9	95	9.30	11.25
10	50	9.60	11.60
11	62	10.00	12.00
12	62	9.94	11.88
13	62	10.00	12.00
14	50	9.60	11.60
15	95	9.30	11.25
16	100	9.00	11.00
17	80	9.88	11.14
18	70	9.41	10.55
19	50	9.60	11.60
20	80	9.88	11.14
Hardness (N)		Thickness (mm)	Length (mm)
Average	= 73.70	Average	= 9.28
Minimum	= 50	Minimum	= 8.12
Maximum	= 100	Maximum	= 10.00
Std. Deviation	= 17.79	Std. Deviation	= 0.63
Result:	Complies	Result:	Complies
Average	= 11.13	Average	= 11.13
Minimum	= 10.25	Minimum	= 10.25
Maximum	= 12.00	Maximum	= 12.00
Std. Deviation	= 0.59	Std. Deviation	= 0.59
Result:	Complies	Result:	Complies

Done by : Mangesh Rane
Date : 27.04.2026