


DISINTEGRATION TEST REPORT

Product Name	TOPIRAMATE 200MG TABLETS USP		
Batch No.	BVN56562	Department	Production
BFG Code No.	BFG-12030	Date	27.04.2026
No. of Samples	6	Std. Disintegration Time (NMT)	00:15:00
Equipment Code No.	SG-136	Disintegration Tester Code No.	DT-809
Media	Purified Water	Side	NA
Temperature Range Jar (°C)	37.0 - 38.1	Temperature Range Bath (°C)	35.5 - 39.5

Test Results

Min. Temperature Jar A (°C)	37.1	Max. Temperature Jar A (°C)	38.0
Min. Temperature Bath (°C)	35.5	Max. Temperature Bath (°C)	39.5
Max. Disintegration Time	00:09:09	Set Bath Temperature	37.2
Mode	Registration	Basket Detail	A
Basket Type	10 Mesh		

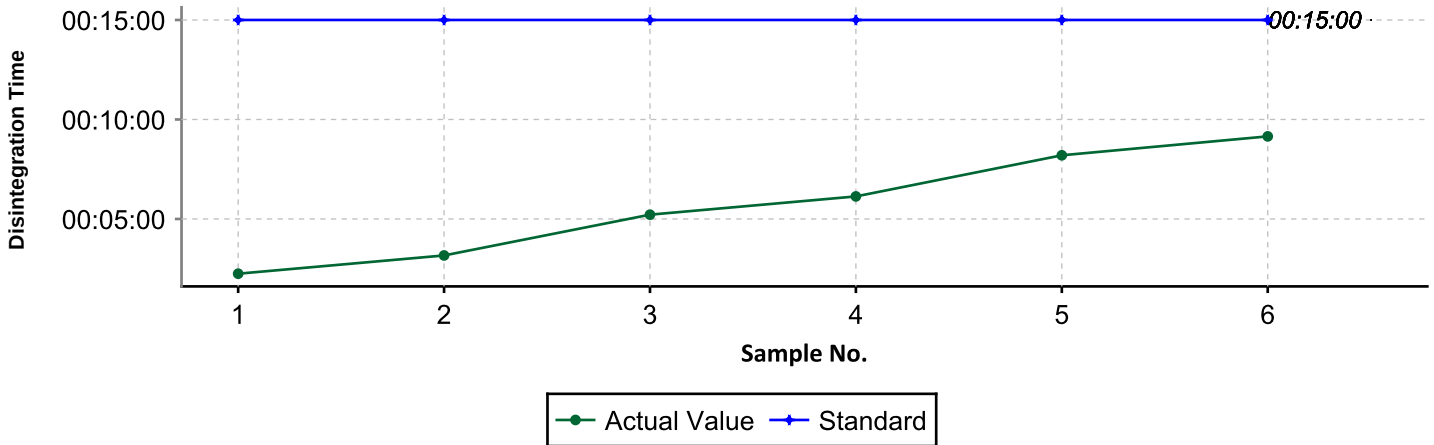

Sample No.	Start Time	End Time	Side	Halt Duration (HH:MM:SS)	Disintegration Time (HH:MM:SS)
1	11:06:28	11:08:43	NA	00:02:00	00:02:15
2	11:06:28	11:09:38	NA	00:02:00	00:03:10
3	11:06:28	11:11:41	NA	00:02:00	00:05:13
4	11:06:28	11:12:36	NA	00:02:00	00:06:08
5	11:06:28	11:14:40	NA	00:02:00	00:08:12
6	11:06:28	11:15:37	NA	00:02:00	00:09:09

Result: Complies**Done by** : Mangesh Rane**Date** : 27.04.2026