


(COMPRESSION) DIAMETER VARIATION RECORD

Product Name	DISPETSIBLE TABLETS 250 MG		
Batch No.	4BA1936	Department	
BFG Code No.	31005657	Date	01.04.2026
No. of Samples	10	Start Time	17:55:15
Equipment Code No.	T-333	Vernier Code No.	T-377
Std Value Diameter (mm)	13.10	Side	NA
Std. Lower Limit (mm)	12.90	Std. Upper Limit (mm)	13.30
Cubicle Name	Compression-3		

Test Results

Average Diameter (mm)	13.11	Standard Deviation	0.09
Minimum Diameter (mm)	12.98	No. of Tablets Below Limit	0
Maximum Diameter (mm)	13.25	No. of Tablets Above Limit	0

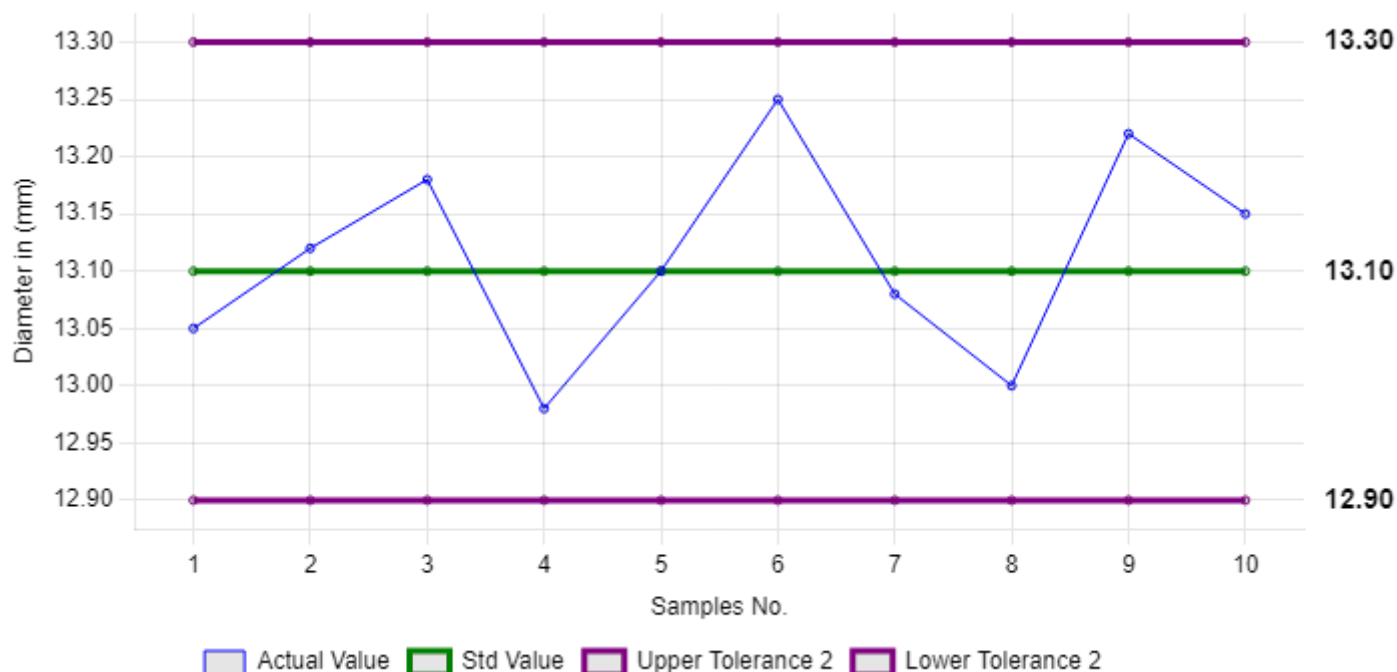

Sample No.	Diameter (mm)	Sample No.	Diameter (mm)	Sample No.	Diameter (mm)	Sample No.	Diameter (mm)	Sample No.	Diameter (mm)	Sample No.	Diameter (mm)
1	13.05	2	13.12	3	13.18	4	12.98	5	13.10	6	13.25
7	13.08	8	13.00	9	13.22	10	13.15				

Result: **Complies**

Performed by: Tushar

Date: 01.04.2026