


REGULAR DISINTEGRATION TEST REPORT

Product Name	captab capsules		
Batch No.	CAP-BT-17	Department	QC
BFG Code No.	bfg-002	Date	05.09.2025
No. of Samples	5	Std. Disintegration Time (NMT)	00:15:00
Equipment Code No.	None	Disintegration Tester Code No.	DT-EDI-2SA
Media	H2O	Side	NA
Temperature Range (°C)	32.0 - 38.0		

Test Results

Min. Temperature (°C)	36.5	Max. Temperature (°C)	37.1
Max. Disintegration Time (HH:MM:SS)	00:15:10	Set Temperature (°C)	37.0
Mode	Dual	Jar Detail	B
Basket Type	10 Mesh		

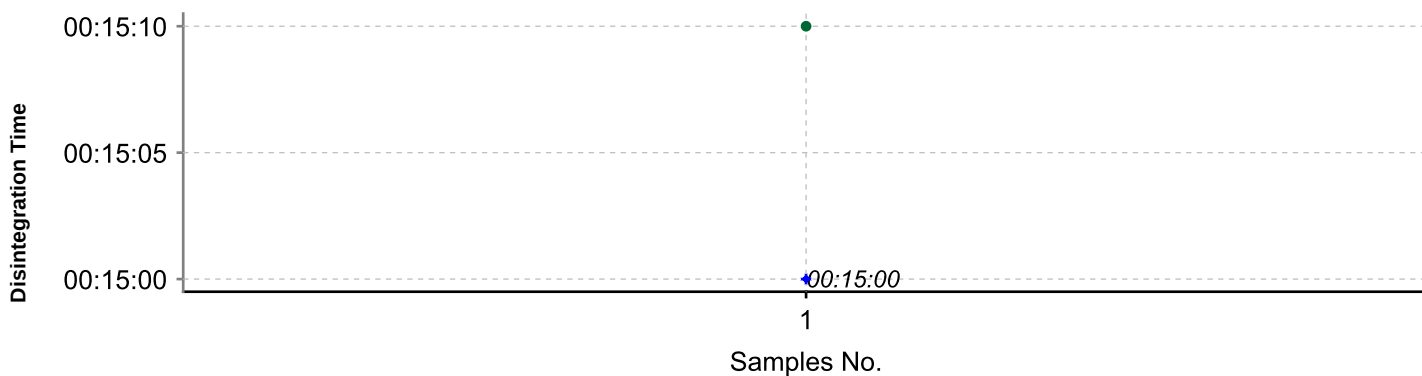

—●— Actual Value —◆— Standard

Sample No.	Start Time	End Time	Side	Halt Duration	Disintegration Time
1	15:00:55	15:16:05	NA	00:00:20	00:15:10

Result: **Not Complies**

Remark: SDFGHJKL234TYUIO34TY

Performed By : kumkum

Checked by : Tantra

Date : 05.09.2025 & 15:00:55

Date : 05.09.2025 & 12:57:40