


REGULAR DISINTEGRATION TEST REPORT

Product Name	PARACETAMOL_50 MG		
Batch No.	IPQC-VAL-REG/D	Department	QC
BFG Code No.	PARA_TAB001	Date	29.08.2025
No. of Samples	6	Std. Disintegration Time (NMT)	00:15:11
Equipment Code No.	None	Disintegration Tester Code No.	DT02
Media	H2O	Side	RHS
Temperature Range (°C)	35.6 - 39.7		

Test Results

Min. Temperature (°C)	37.1	Max. Temperature (°C)	37.7
Max. Disintegration Time (HH:MM:SS)	00:01:39	Set Temperature (°C)	37.0
Mode	Dual	Jar Detail	B
Basket Type	NA		

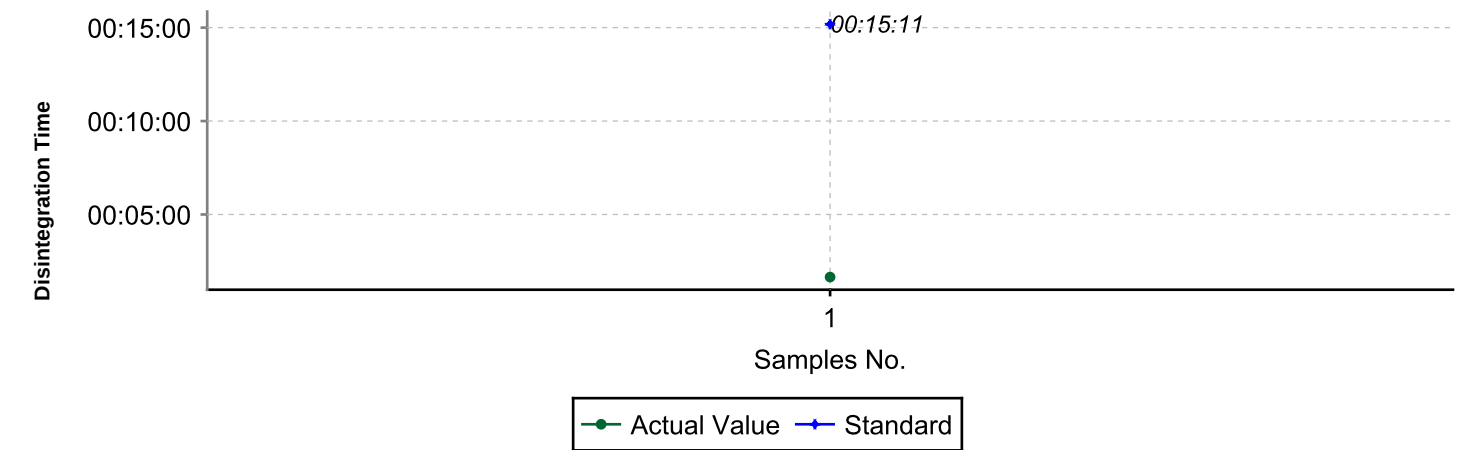

Sample No.	Start Time	End Time	Side	Halt Duration	Disintegration Time
1	12:21:18	12:22:57	RHS	00:00:00	00:01:39

Result: **Complies**

Remark: dfgnm

Performed By : kumkum

Date : 29.08.2025 & 12:21:18

Checked by : Tantra

Date : 29.08.2025 & 12:51:46