


REGULAR DISINTEGRATION TEST REPORT

Product Name	Hydrachloride 500mg IP Capsule		
Batch No.	BT_07_Test	Department	QC
BFG Code No.	1411	Date	09.10.2024
No. of Samples	7	Std. Disintegration Time (NMT)	00:15:00
Equipment Code No.	None	Disintegration Tester Code No.	ED-3PO
Media	H2O	Side	NA
Temperature Range (°C)	35.0 - 39.0		

Test Results

Min. Temperature (°C)	34.6	Max. Temperature (°C)	34.6
Max. Disintegration Time	00:10:20	Set Temperature (°C)	39.2
Mode	NA	Jar Detail	C
Basket Type	10 Mesh		

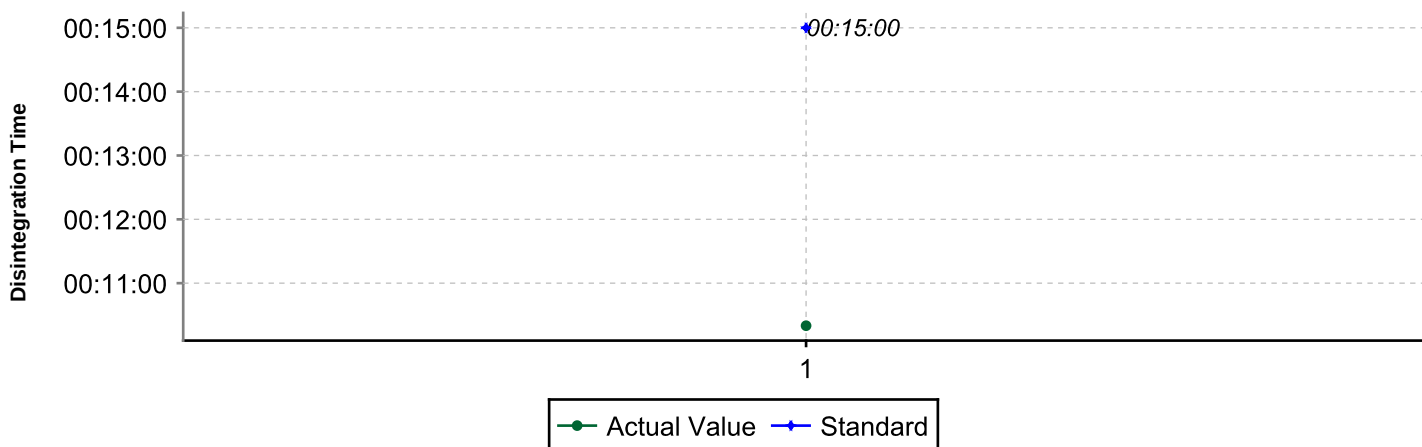

Sample No.	Start Time	End Time	Side	Halt Duration	Disintegration Time
1	14:59:59	15:10:19	NA	00:04:27	00:10:20

Result: **Not Complies**

For testing

Performed By : Abhishek
Date : 09.10.2024Checked by : Sail
Date : 09.10.2024