


REGULAR DISINTEGRATION TEST REPORT

Product Name	PARACETAMOL_50 MG		
Batch No.	Double-001	Department	QA
BFG Code No.	PARA_TAB001	Date	05.09.2025
No. of Samples	7	Std. Disintegration Time (NMT)	00:15:11
Equipment Code No.	Equipment-1	Disintegration Tester Code No.	DT-EDI-2SA
Media	WATER	Side	RHS
Temperature Range (°C)	35.6 - 39.7		

Test Results

Min. Temperature (°C)	37.2	Max. Temperature (°C)	37.7
Max. Disintegration Time (HH:MM:SS)	00:01:19	Set Temperature (°C)	37.1
Mode	Dual	Jar Detail	B
Basket Type	10 Mesh		

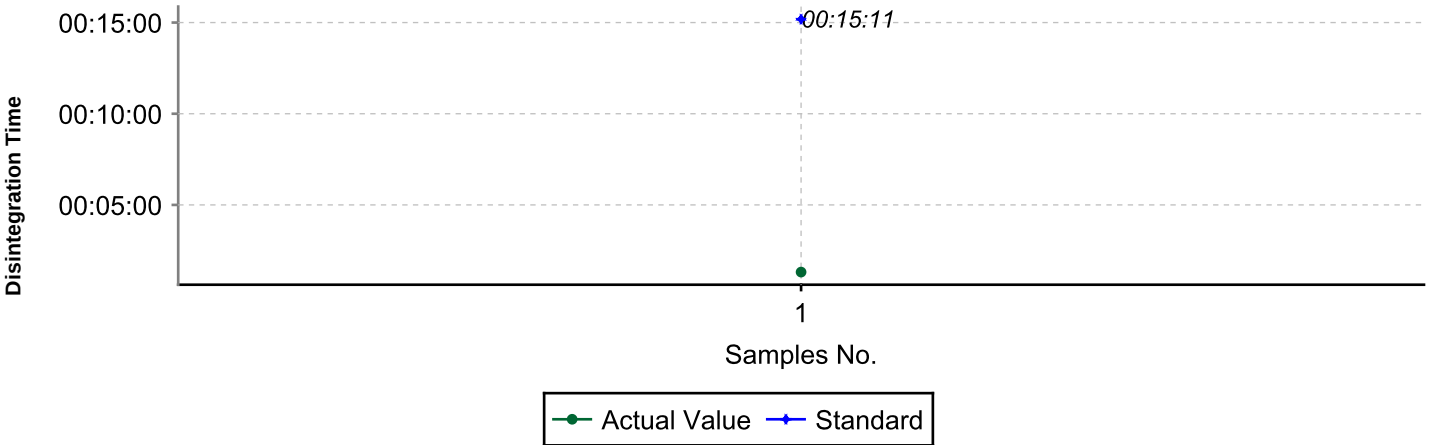

Sample No.	Start Time	End Time	Side	Halt Duration	Disintegration Time
1	15:03:19	15:04:38	RHS	00:01:12	00:01:19

Result: **Complies**

Performed By : kuldeep
Date : 05.09.2025 & 15:03:19