


REGULAR DISINTEGRATION TEST REPORT

Product Name	Azithromicine tab 50 mg		
Batch No.	BT-DT-Com01	Department	QC
BFG Code No.	BFG-11332	Date	07.10.2025
No. of Samples	5	Std. Disintegration Time (NMT)	00:15:00
Equipment Code No.	EQ001	Disintegration Tester Code No.	DT-EDI-2SA
Media	WATER	Side	RHS
Temperature Range (°C)	34.0 - 39.0		

Test Results

Min. Temperature (°C)	37.8	Max. Temperature (°C)	38.6
Max. Disintegration Time (HH:MM:SS)	00:14:59	Set Temperature (°C)	37.2
Mode	Dual	Jar Detail	B
Basket Type	10 Mesh		

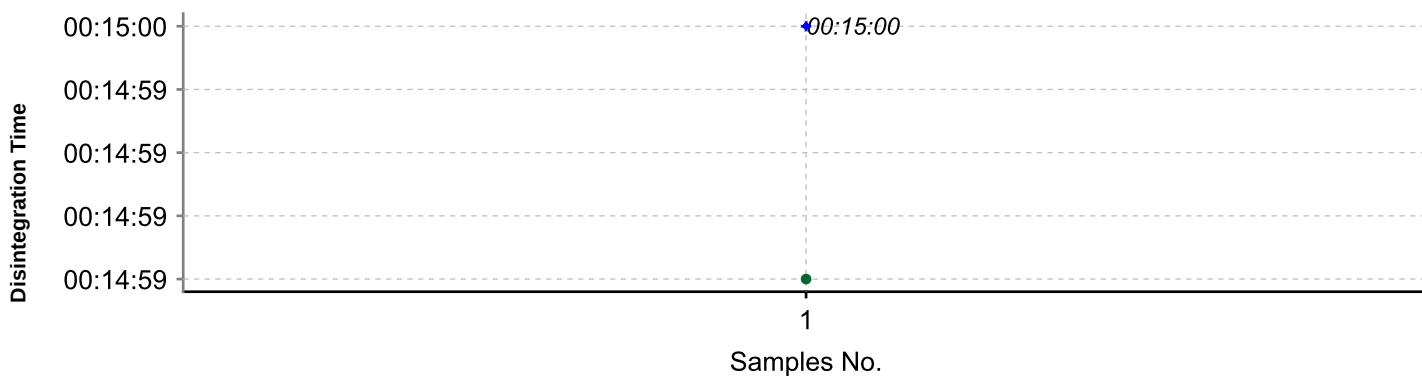

—●— Actual Value —●— Standard

Sample No.	Start Time	End Time	Side	Halt Duration	Disintegration Time
1	15:05:26	15:20:25	RHS	00:00:00	00:14:59

Result: **Complies**

Remark: test

Performed By : Mangesh

Checked by : Devendra

Date & Time : 07.10.2025 & 15:05:26

Date & Time : 07.10.2025 & 16:17:10