


REGULAR DISINTEGRATION TEST REPORT

Product Name	PARACETAMOL_50 MG		
Batch No.	IPQCDT2COA-1065	Department	QC
BFG Code No.	PARA_TAB001	Date	05.09.2025
No. of Samples	5	Std. Disintegration Time (NMT)	00:15:11
Equipment Code No.	EQ 1	Disintegration Tester Code No.	DT-EDI-2SA
Media	WATER	Lot No.	21
Temperature Range (°C)	35.6 - 39.7		

Test Results

Min. Temperature (°C)	36.5	Max. Temperature (°C)	37.0
Max. Disintegration Time (HH:MM:SS)	00:00:34	Set Temperature (°C)	37.0
Mode	Dual	Jar Detail	A
Basket Type	10 Mesh		

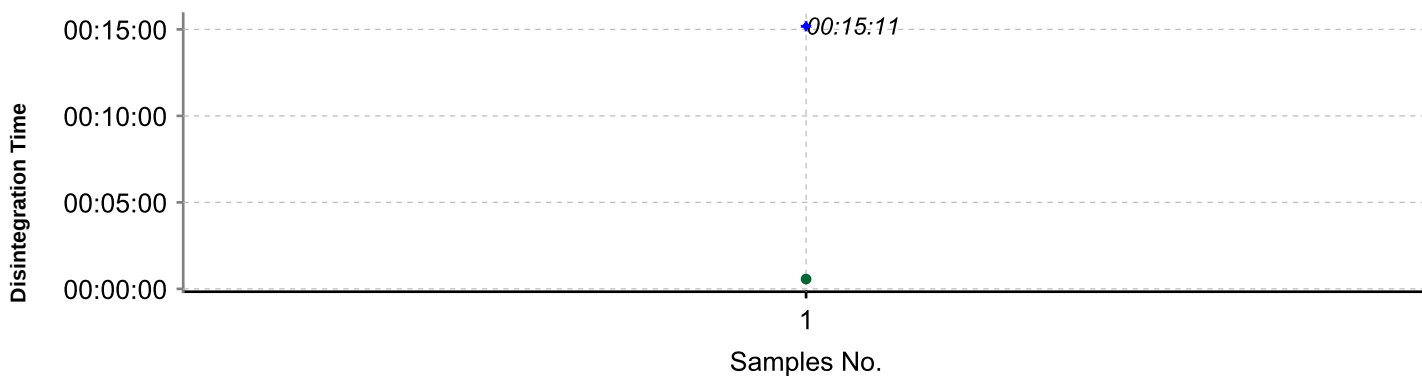

—●— Actual Value —●— Standard

Sample No.	Start Time	End Time	Side	Halt Duration	Disintegration Time
1	14:50:13	14:50:47	NA	00:00:10	00:00:34

Result: **Complies**

Remark: TEST

Performed By : kuldeep

Checked by : Mangesh

Date & Time : 05.09.2025 & 14:50:13

Date & Time : 05.09.2025 & 14:25:33